Assembly Notes

1.After opening the carton, please carefully check for missing parts and transportation damage and if needed, contact dealer immediately.
2.Once installed, the gas lift will be difficult to remove. It is not recommended to remove the lift to avoid damage to other parts of the chair.
3.Contact dealer if disassembly assistance is needed.

Usage Notes

1.Intended for use indoors.
2.Intended for single person use.
3.Do not sit on end of chair to avoid accidental tipping and injury.
4.Do not step or stand on the chair – chair is intended for sitting only.
5.Use caution when reclining, especially as tension is reduced by user.
6.Do not lean against product – chair is intended for sitting only.
7.Avoid contact with sharp objects, heavy tools, and hot surfaces.
8.As assembly may loosen overtime, for best user safety, conduct regular check of nuts and bolts to insure they are always tight and secure.
9.To clean, wipe with a soft and dry cleaning cloth. If there are stains on fabric, use a mild detergent to wipe clean and let it air dry.








Model#: 602MMFBK/603MMFGT
Name: Oslo
Description: Mid-Back Mesh Task Chair
Color: Black/Light Gray

Assembly Instructions &User manual




Please read the instruction sheets completely before assembly.


Assembly Instructions

A  Seat x1	 Backrest x1	C  Armrest x1	D  Mechanism x1
E  Gas lift x1	F  Nylon Base x1	G  Caster x5	⑥  Allen Key x1
①  1/4"*1-1/4" with washer x6	②  M8*20 x4	③  M8*25 x3	④  Spring washer x3
			⑤  Flat washer x3

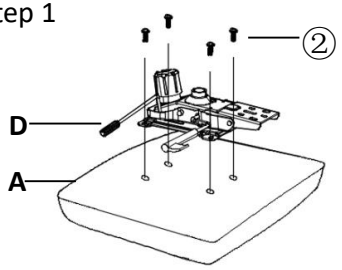
Step 1



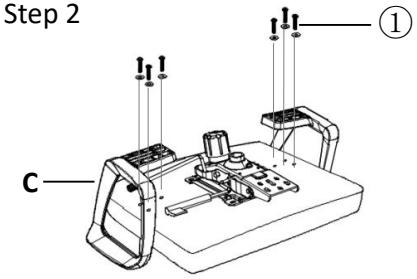
Step 2



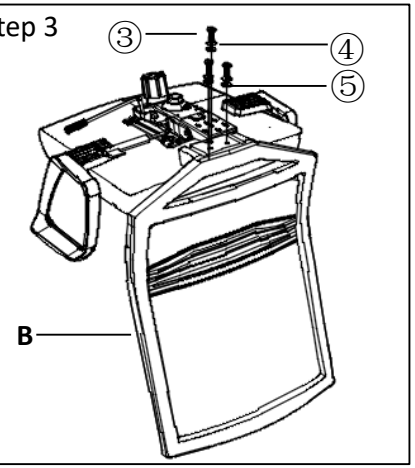Step 3



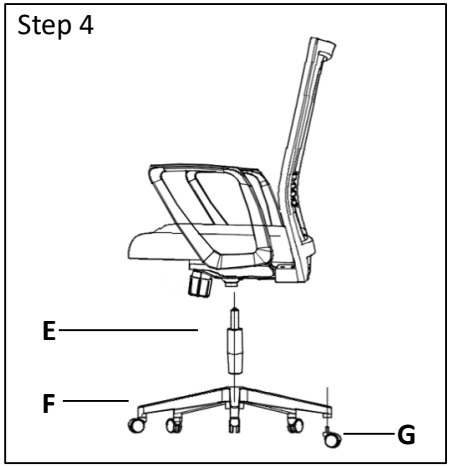Step 4



Tilt angle adjustable Backrest
Push the lever to lock the tilt angle of backrest,
Pull the lever to unlock the backrest and allow the chair to recline.

Seat height adjustment
Pull the lever upward to adjust the seat height up and down.

Seat depth adjustment
Pull the lever upward to adjust the seat depth.



Height adjustable Lumbar support

Tension tilt adjustable
Rotating the knob to adjust the tilting tension according tc different weight requires.